# Wagner Cone Prosthesis® Hip Stem


Ordering Information

## Implants



Wagner Cone Prosthesis 125° Hip Stem


Protasul-64 Alloy
Taper 12/14
Uncemented

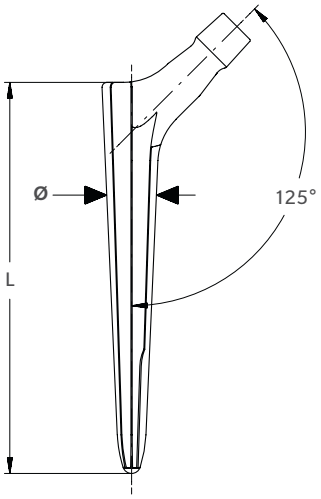




Wagner Cone Prosthesis 135° Hip Stem

Protasul-64 Alloy
Taper 12/14
Uncemented

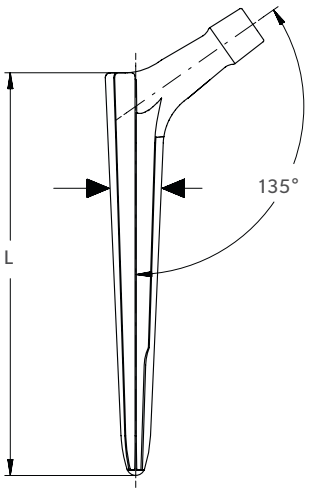


STERILE R

| Ø mm | L mm | Size | REF |
|---|---|---|---|
| 13 | 115.0 | 27.5 | 01.00561.213 |
| 14 | 125.5 | 31.7 | 01.00561.214 |
| 15 | 125.7 | 32.5 | 01.00561.215 |
| 16 | 125.9 | 33.4 | 01.00561.216 |
| 17 | 126.2 | 34.2 | 01.00561.217 |
| 18 | 126.4 | 35 | 01.00561.218 |
| 19 | 126.6 | 35.9 | 01.00561.219 |
| 20 | 126.8 | 36.7 | 01.00561.220 |
| 21 | 127.0 | 37.5 | 01.00561.221 |
| 22 | 127.2 | 38.3 | 01.00561.222 |
| 23 | 127.4 | 39.2 | 01.00561.223 |
| 24 | 127.6 | 40 | 01.00561.224 |

STERILE R

| Ø mm | L mm | Size | REF |
|---|---|---|---|
| 13 | 115.0 | 26.2 | 01.00561.313 |
| 14 | 125.5 | 29.7 | 01.00561.314 |
| 15 | 125.7 | 30.4 | 01.00561.315 |
| 16 | 125.9 | 31.1 | 01.00561.316 |
| 17 | 126.2 | 31.8 | 01.00561.317 |
| 18 | 126.4 | 32.5 | 01.00561.318 |
| 19 | 126.6 | 33.2 | 01.00561.319 |
| 20 | 126.8 | 33.9 | 01.00561.320 |
| 21 | 127.0 | 34.7 | 01.00561.321 |
| 22 | 127.2 | 35.4 | 01.00561.322 |
| 23 | 127.4 | 36.1 | 01.00561.323 |
| 24 | 127.6 | 36.8 | 01.00561.324 |


# Instruments



| Product | REF |
|---|---|
| Tray for Wagner Cone Prosthesis Instruments (complete) | ZS01.00369.010 |
| Tray base for Wagner Cone Prosthesis Instruments (empty) | 01.00369.011 |
| Tray insert for Wagner Cone Prosthesis Instruments (empty) | 01.00369.012 |
| Standard tray cover, grey | 01.00029.031 |



| Product | REF |
|---|---|
| Handle with quick coupling | 75.00.25 |

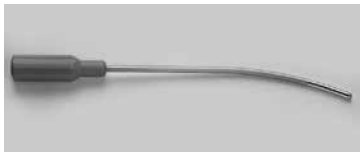

| Product | REF |
|---|---|
| Gauge for the medullary cavity | 75.11.40-01 |




| Product | REF |
|---|---|
| Extractor for Wagner Cone Prosthesis Stem | 75.11.00-09 |



| Product | REF |
|---|---|
| Reamer | 75.00.25 |



| Product | REF |
|---|---|
| Impactor | 75.11.15-01 |

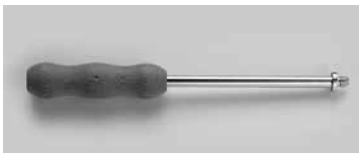

| Product | REF |
|---|---|
| Reduction Lever | 75.01.38 |

| Ø mm | REF |
|---|---|
| 13 | 75.11.15-130 |
| 14 | 75.11.15-140 |
| 15 | 75.11.15-150 |
| 16 | 75.11.15-160 |
| 17 | 75.11.15-170 |
| 18 | 75.11.15-180 |
| 19 | 75.11.15-190 |
| 20 | 75.11.15-200 |
| 21 | 75.11.15-210 |
| 22 | 75.11.15-220 |
| 23 | 75.11.15-230 |
| 24 | 75.11.15-240 |

# **Instruments** - Upon request



| Product | Ø Size | REF |
|---|---|---|
| Repositioning tops | 22 mm | 78.00.38-22 |
| | 28 mm | 78.00.38-28 |
| | 32 mm | 78.00.38-32 |




| Product | Ø Size | REF |
|---|---|---|
| Calcar rasp | - | 71.00.92 |



| Product | Ø Size | REF |
|---|---|---|
| Trial heads | 22 12/14 S | 73.11.22-05 |
| | 22 12/14 M | 73.11.22-06 |
| | 22 12/14 L | 73.11.22-07 |
| | 28 12/14 S | 01.01559.128 |
| | 28 12/14 M | 01.01559.228 |
| | 28 12/14 L | 01.01559.328 |
| | 32 12/14 S | 01.01559.132 |
| | 32 12/14 M | 01.01559.232 |
| | 32 12/14 L | 01.01559.332 |



| Product | Ø Size | REF |
|---|---|---|
| Trial heads | 28 12/14 XL | 01.01559.428 |
| | 32 12/14 XL | 01.01559.432 |
| | 36 12/14 S | 01.01559.136 |
| | 36 12/14 M | 01.01559.236 |
| | 36 12/14 L | 01.01559.336 |
| | 36 12/14 XL | 01.01559.436 |

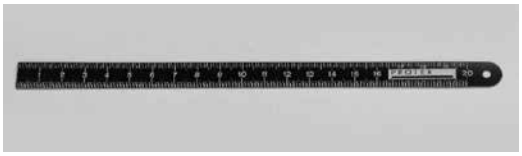

| Product | Ø Size | REF |
|---|---|---|
| Ruler 20 cm | - | 95.00.03 |



| Product | Ø Size | REF |
|---|---|---|
| Repositioning top | 36 mm | 78.00.38-36 |



| Product | Ø Size | REF |
|---|---|---|
| AO Adaptor/ TPP Adaptor | - | 5637 |

**References**


1. H. Wagner and M. Wagner. Cone Prosthesis for the Hip Joint. Archives Orthopaedic and Trauma Surgery. 120(1-2): 88–95,2000.
2. C. C. Castelli, *et al*. Radiographic Evaluation of the "Conus" Uncemented Stem. Hip International. Lit. No. 06.00704.012x 9(3): 133-8, 1999.
3. Y. Y. Kim *et al*. Total Hip Reconstruction in the Anatomically Distorted Hip – Cemented Versus Hybrid Total Hip Arthroplasty. Archives Orthopaedic and Trauma Surgery. 117(1): 8–14, 1998.



This documentation is intended exclusively for physicians and is not intended for laypersons. Information on the products and procedures contained in this document is of a general nature and does not represent and does not constitute medical advice or recommendations. Because this information does not purport to constitute any diagnostic or therapeutic statement with regard to any individual medical case, each patient must be examined and advised individually, and this document does not replace the need for such examination and/or advice in whole or in part.

Please refer to the package inserts for important product information, including, but not limited to, contraindications, warnings, precautions, and adverse effects.

Copyright 2006–2016 by Zimmer GmbH Printed in Switzerland Subject to change without notice

©2016 Zimmer Biomet


ZIMMER BIOMET

Your progress. Our promise.™


0623.1-EMEA-en REV0516 A4